

H
QC
807.5
Uo
Ho
no.92
c.2

NOAA Technical Memorandum ERL WPL-92



FREQUENCY RESPONSE MEASUREMENTS
ON LYMAN-ALPHA HUMIDIOMETERS

J. T. Priestley
W. D. Cartwright

Wave Propagation Laboratory
Boulder, Colorado
February 1982

noaa

NATIONAL OCEANIC AND
ATMOSPHERIC ADMINISTRATION

/ Environmental Research
Laboratories

QC
807.5
U6W6
no. 92
c.2

NOAA Technical Memorandum ERL WPL-92

FREQUENCY RESPONSE MEASUREMENTS
ON LYMAN-ALPHA HUMIDIOMETERS

J. T. Priestley
W. D. Cartwright

Partial support for this project was provided
by the U.S. Army Research Office

Wave Propagation Laboratory
Boulder, Colorado
February 1982

CENTRAL
LIBRARY

JUL 1 1982

N.O.A.A.
U. S. Dept. of Commerce



UNITED STATES
DEPARTMENT OF COMMERCE

Malcolm Baldrige,
Secretary

NATIONAL OCEANIC AND
ATMOSPHERIC ADMINISTRATION

John V. Byrne,
Administrator

Environmental Research
Laboratories

George H. Ludwig
Director

82 01406

NOTICE

Mention of a commercial company or product does not constitute an endorsement by NOAA Environmental Research Laboratories. Use for publicity or advertising purposes of information from this publication concerning proprietary products or the tests of such products is not authorized.

CONTENTS

| | PAGE |
|--|------|
| ABSTRACT | 1 |
| 1. The Problem | 1 |
| 2. Results | 2 |
| 3. Humidiometer Comparisons | 2 |
| 4. An Improved Detector Amplifier Design | 4 |
| 5. Conclusions | 4 |
| 6. Acknowledgments | 4 |
| REFERENCES | 5 |

FREQUENCY RESPONSE MEASUREMENTS ON LYMAN-ALPHA HUMIDIOMETERS

J. T. Priestley and W. D. Cartwright

NOAA/ERL/Wave Propagation Laboratory
Boulder, Colorado 80303

The primary instrument used for measuring high-frequency humidity fluctuations is the Lyman-alpha humidiometer; yet, there is virtually no published data on its frequency response. Attempting to fill this void, both amplitude and phase measurements were made on several such instruments. These measurements showed frequency responses (amplitude 3 dB down) ranging from approximately 160 to 800 Hz. Measurements of a specially modified unit showed no fundamental frequency limitation up to at least 10 kHz.

1. THE PROBLEM

During the summer of 1981, William Kohsieck, a visiting fellow from the Royal Netherlands Meteorological Institute, made a series of simultaneous temperature/humidity measurements in the boundary layer. The temperature sensor was a 2- μ -diameter platinum wire, and the humidity sensor was a Lyman-alpha humidiometer. The results of spectral and cross-spectral analysis of the data indicated a consistent and unexplained anomaly starting at about 20 Hz and gradually increasing toward 100 Hz, the highest frequency analyzed. In the power spectra, the anomaly was a more rapid drop-off in the humidity spectra than that in the temperature spectra. (At 50 Hz the humidity was down about 3 dB compared with the temperature.) In the phase spectra, the anomaly was a systematic phase difference between temperature and humidity going from almost no mismatch at 20 Hz to an approximately 180° mismatch at 100 Hz.

Upon further investigation, we found that very little data were available on the frequency response characteristics of Lyman-alpha humidiometers, in spite of the fact that the Lyman-alpha humidiometer is essentially the only fast-response humidity-measuring instrument currently available. Tillman (1965), in describing the nitric oxide photoionization detector (as used in all of the Lyman-alpha humidiometers investigated in this report), states, "The response time of this detector is presently unknown but probably is on the order of 0.001 seconds." Buck (1976), in describing a Lyman-alpha humidiometer developed at the National Center for Atmospheric Research, states that its response time is 12 ms. He does not indicate the cause of this particular response time nor how it was measured. The only actual response curves we found were in an unpublished report by Friehe (1978). His results are discussed in Section 3 of this report.

In the hope of resolving the immediate problem, as well as achieving a better understanding of the Lyman-alpha humidiometer frequency response characteristics for future users, we made amplitude/phase response measurements of a number of existing instruments, and of one that we modified.

2. RESULTS

We conclude from our measurements that the anomaly in Kohsieck's data was not caused by the frequency response of his Lyman-alpha humidiometer; the frequency response of his humidiometer corresponded to that of a simple RC filter up to the 3-dB point of 490 Hz.

All of the other Lyman-alpha humidiometers that we tested, except one, had 3-dB cut-off frequencies between 160 and 800 Hz, and appeared to be limited by their detector amplifiers. The one exception was a humidiometer for which we built an extended-range detector amplifier. It had a frequency response extending beyond 10 kHz, which is important because it shows that there is no fundamental limitation, at least up to 10 kHz, in the response of Lyman-alpha humidiometers. A response to 10 kHz may be desirable for aircraft-mounted instruments.

3. HUMIDIOMETER COMPARISONS

The experimental arrangement is shown in Fig. 1. The Lyman-alpha source was modulated with a sine wave of approximately 10 to 15 v (peak-to-peak amplitude) and the observed signal was taken from the detector amplifier. Particular attention had to be exercised in the way the reference signal was derived. Taking the reference signal directly from the oscillator output would have required an excessively large blocking capacitor C_1 , because of the relatively low and ill-defined AC impedance of the Lyman-alpha source. With the circuit as shown in Fig. 1, the capacitor C_2 sees the relatively high and well-defined impedance (.5 MΩ) of the scope and phase meter in parallel. This causes a worst-case error of approximately 0.1% in amplitude and 2° in phase. (The worst-case error occurs at the lowest frequency measured, 20 Hz.)

The humidiometer used by Kohsieck was tested using the above procedure. The resulting response curves, along with the circuit diagram of the detector amplifier, are shown in Fig. 2. The 3-dB amplitude point occurs at 490 Hz. The phase at this point is 45°; thus, below the cut-off frequency $f_c = 490$ Hz, the response appears to behave like a simple RC filter with a time constant

$$\tau = \frac{1}{2\pi f_c} = 0.325 \text{ ms}$$

We note from Fig. 2 that the 100-MΩ resistor and the 3-pF capacitor in the feedback loop correspond to a simple RC filter with a time constant $\tau = 0.3$ ms. The slightly larger time constant from the response curves is easily accounted for by component tolerance and stray capacitance on the circuit board. In the 1000- to 2000-Hz region, the response curves depart from those of a simple RC filter: the amplitude response curve falls off more rapidly than 6 dB per octave, and the phase response does not asymptotically approach 90°. This departure is probably caused by the intrinsic frequency characteristics of the op-amp.

When we compare the results of Fig. 2 (no perceptible roll-off at 50 Hz and a 12° phase shift at 100 Hz) with the unexplained anomaly in Kohsiek's experimental data (a 3-dB roll-off at 50 Hz and a 180° phase shift at 100 Hz), it is evident that the frequency response of the hygrometer is not the explanation.

We obtained two Lyman-alpha hygrometers from the Boulder Atmospheric Observatory (Model LA-3 made by the Research Systems Facility of the National Center for Atmospheric Research). The critical part of the detector amplifiers and the response curves for one of the instruments are shown in Fig. 3; the response curve of the other was very similar. The 3-dB amplitude point, as well as the 45° phase point, are close to 150 Hz, which closely corresponds to the cut-off frequency expected from the components in the feedback loop of the op-amp.

$$f_c = \frac{1}{2\pi RC} = 159 \text{ Hz}$$

Arden Buck, of the National Center for Atmospheric Research, loaned us a two-channel experimental Lyman-alpha hygrometer. Fig. 4 shows the response curves and the detector amplifier schematic for channel 1, and Fig. 5 gives similar information for channel 2. (Note the difference in feedback resistors.) The large peak in each of the amplitude response curves is apparently caused by the presence of capacitor C_2 .*

Friehe (1978), made response measurements, similar to those made here, on a commercial (ERC Company) Lyman-alpha hygrometer and also on a modified version with a specially designed, improved, detector amplifier. He found the 3-dB cut-off points to be 1.7 kHz and 3.6 kHz, respectively. Although his modified version was an improvement over the commercial version, he apparently expected a greater improvement because he concluded the response was limited by some fundamental property of the photo-detector.

* Capacitors C_1 and C_2 , as well as the 10- $k\Omega$ resistor, are part of a gain-switching network. The schematic diagrams in Figs. 4 and 5 show the configuration used in the present measurements (it corresponds to the lowest gain setting).

4. AN IMPROVED DETECTOR AMPLIFIER DESIGN

We now approached the problem of Lyman-alpha frequency response a little differently: instead of asking what was available, we asked what would we like to have available. From this viewpoint we assumed that we wanted to measure scale sizes down to 1 cm (the physical size limitation of current Lyman-alphas) from an aircraft flying at 100 m s^{-1} . This translates into a frequency response requirement in the order of 10 kHz, significantly exceeding that of the best instrument measured to date.

At this point, we wanted to know if the frequency response was limited by some fundamental characteristic of the photo-detector, for example, the finite drift velocity of positive ions toward the cathode. Attempting to resolve this question, we built a new detector amplifier and substituted it into channel 1 of Buck's humidiometer. The resulting response (Fig. 6) extended to 10 kHz, with less than a 2-dB variation in amplitude and 10° variation in phase.

5. CONCLUSIONS

The primary conclusions are that the anomaly in Kohsieck's data was not caused by the Lyman-alpha humidiometer, and that, with proper design, the frequency response of these instruments can be extended to at least 10 kHz. Any fundamental limitations that may exist are beyond that.

6. ACKNOWLEDGMENTS

We are indebted to A. Buck for his encouragement as well as for the loan of an experimental Lyman-alpha humidiometer. We also gratefully acknowledge the helpful discussions with C. Friehe.

REFERENCES

Buck, A. L., 1976. The variable-path Lyman-alpha hygrometer and its operating characteristics. Bulletin of the American Meteorological Society, Vol. 57, No. 9, 1113-1118.

Friehe, C. A., 1978. Performance of the Lyman-alpha hygrometer. (Unpublished at this time but may be published in 1982 as a technical memorandum by the National Center for Atmospheric Research, Boulder, Colorado.)

Tillman, J. E., 1965. Water vapor density measurements utilizing the absorption of vacuum ultraviolet and infrared radiation. In Humidity and Moisture, Measurement and Control in Science and Industry, Vol. 1, Principles and Methods of Measuring Humidity in Gases, R. E. Ruskin, Ed., Reinhold, New York, 428-443.

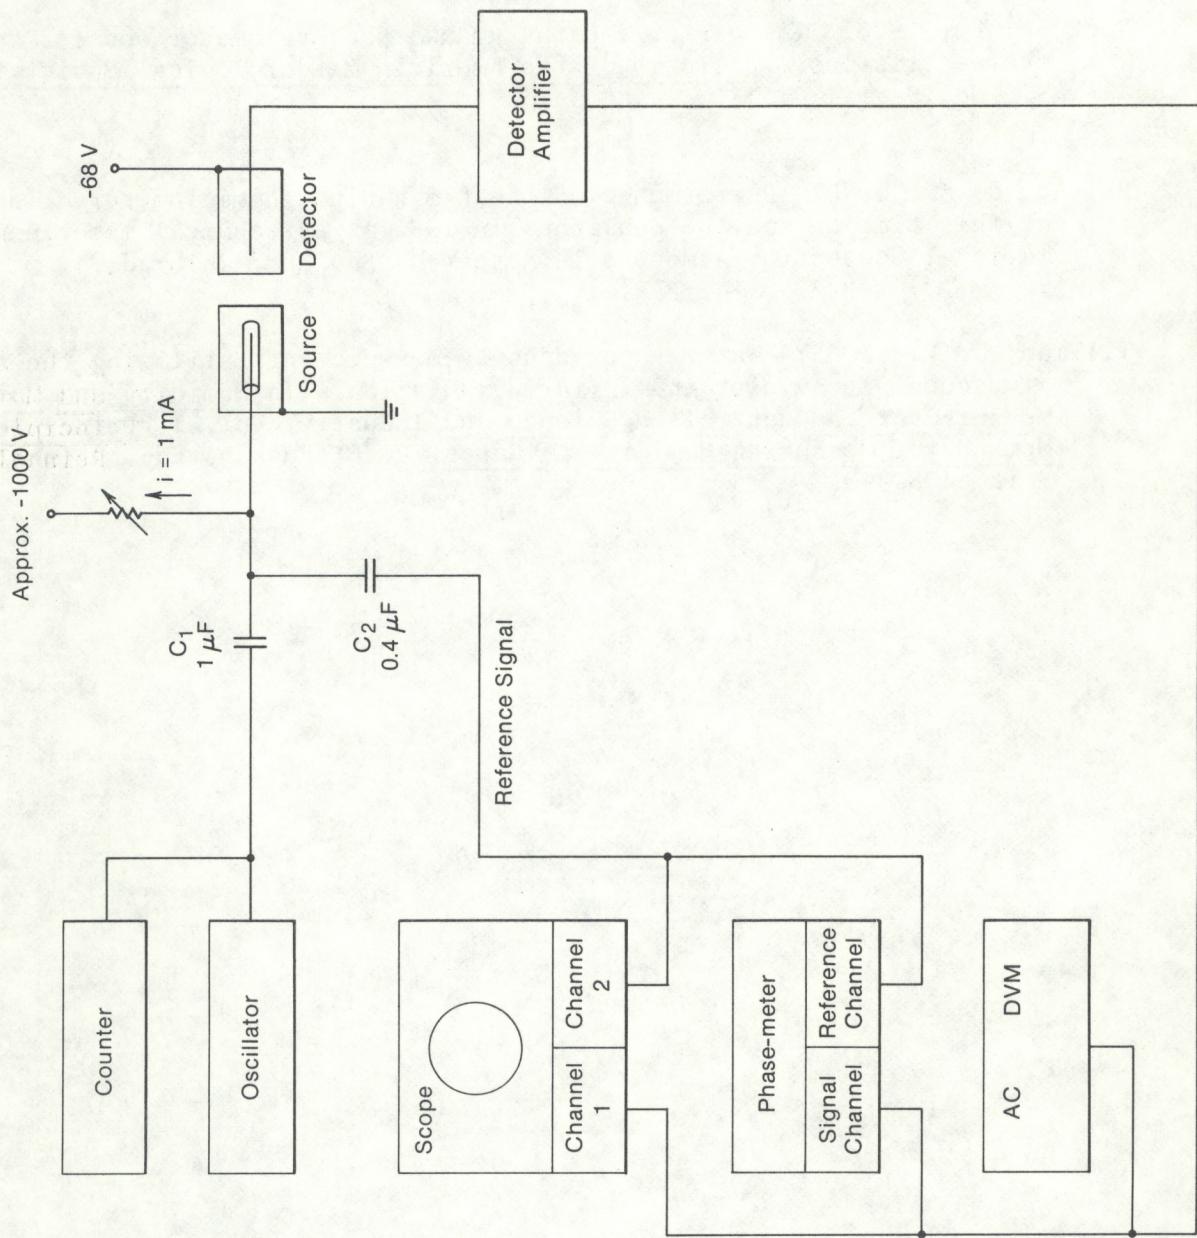


Fig. 1.--Experimental arrangement for Lyman-alpha frequency response measurements.

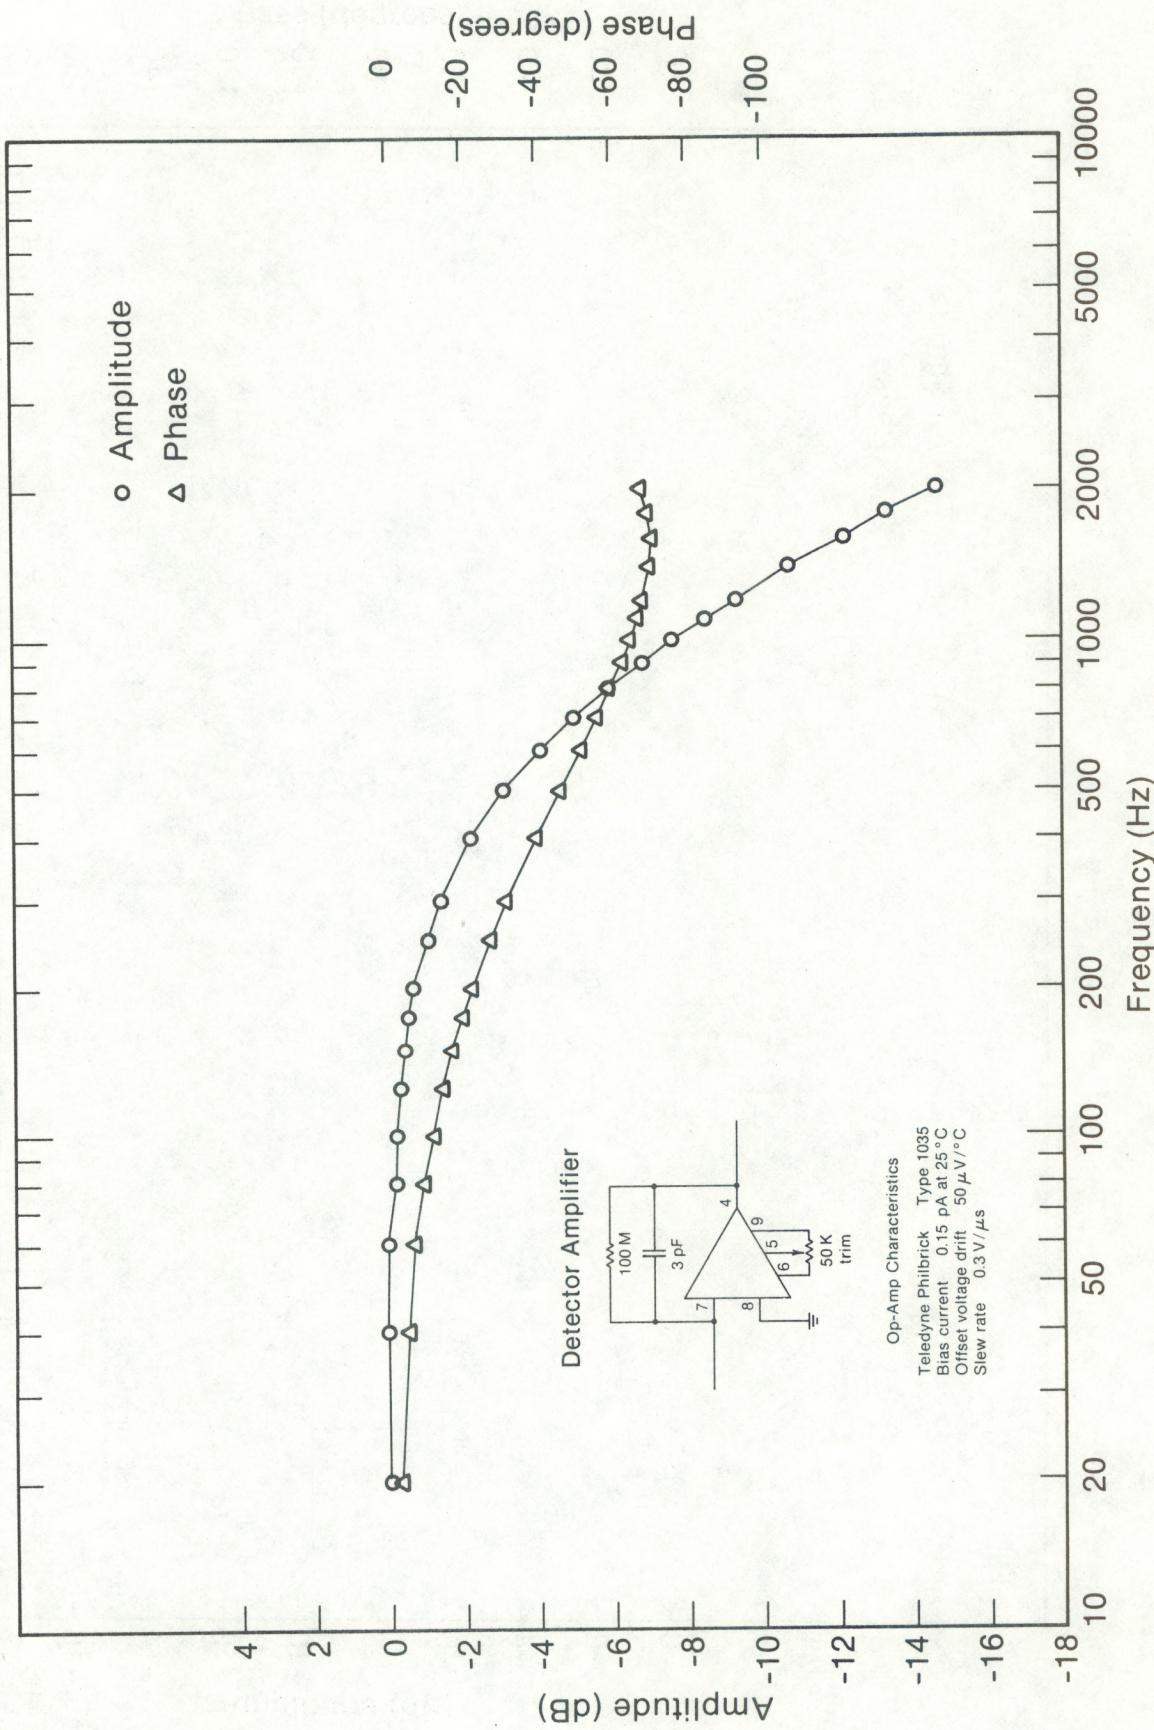


Fig. 2.—Amplitude and phase response of Kohsiek's humiditymeter.

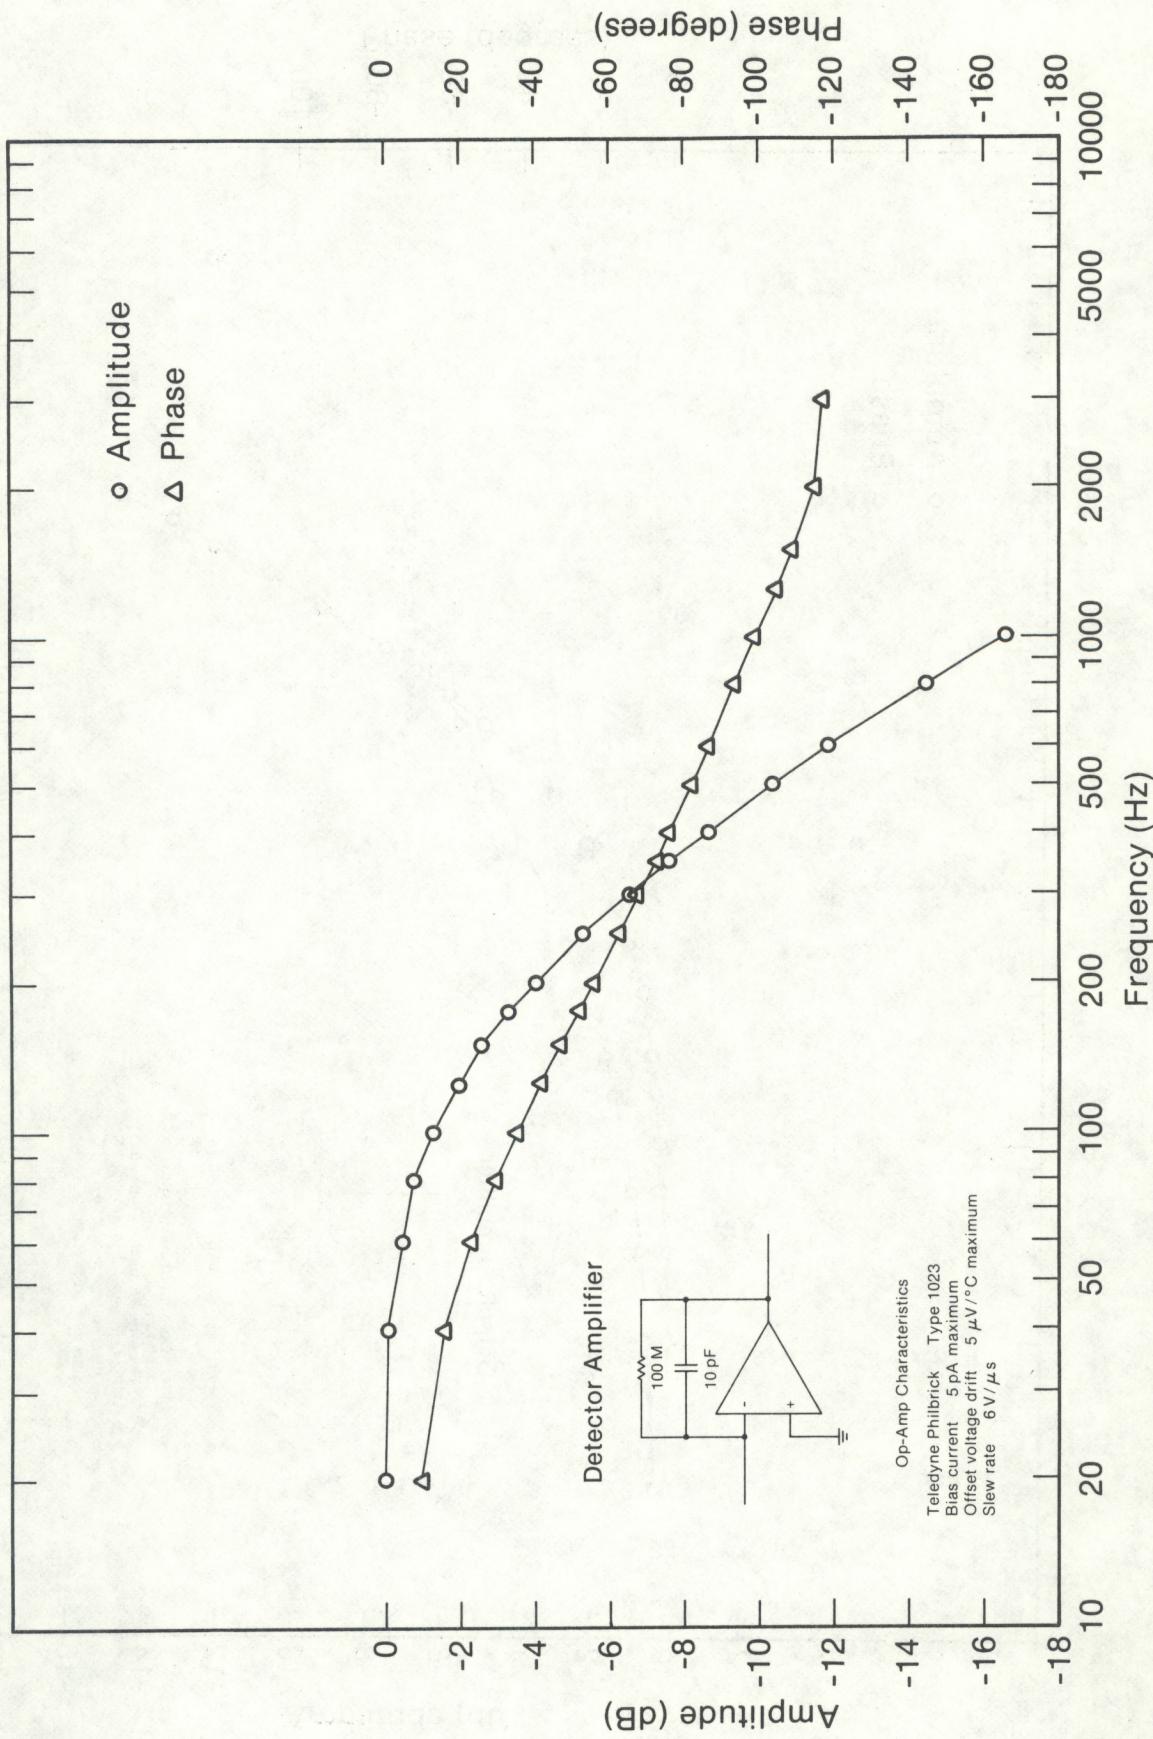


Fig. 3.—Amplitude and phase response of a model LA-3 humidometer used by the Boulder Atmospheric Observatory.

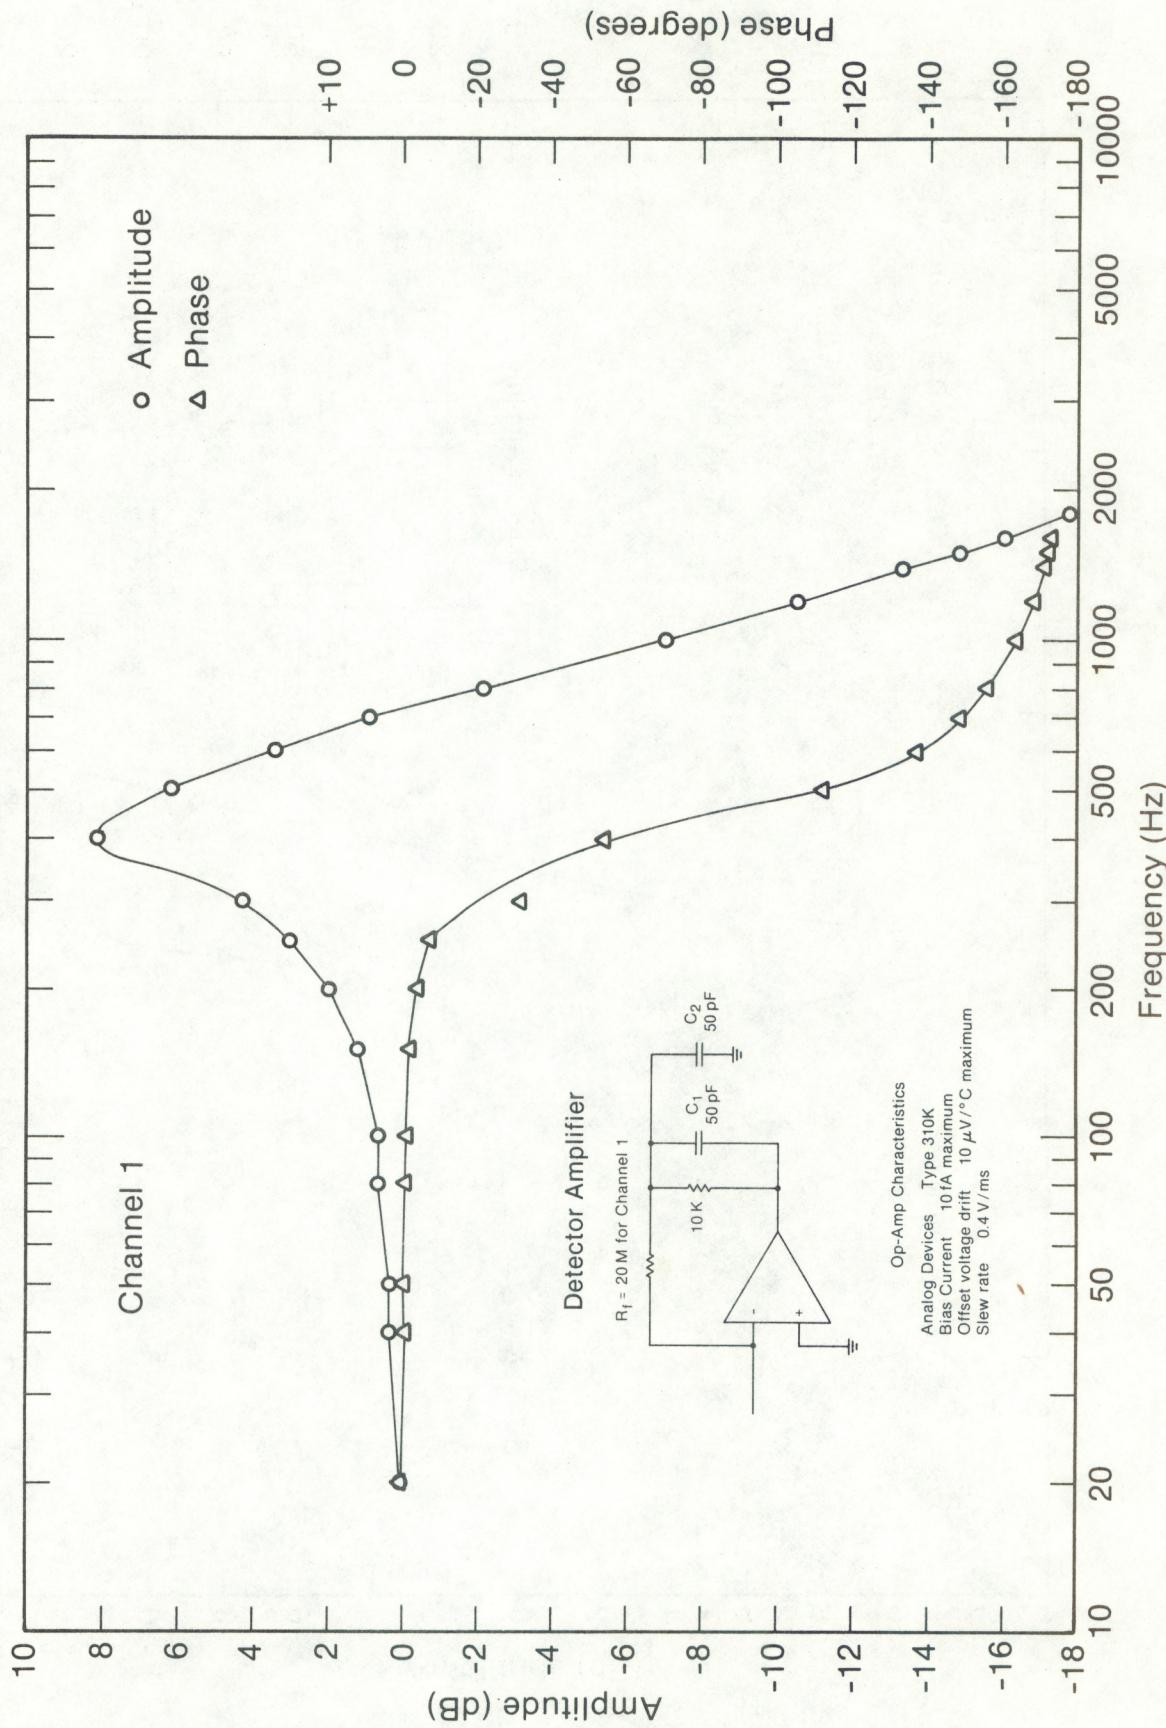


Fig. 4.—Amplitude and phase response of channel 1 of Buck's experimental humidilometer.

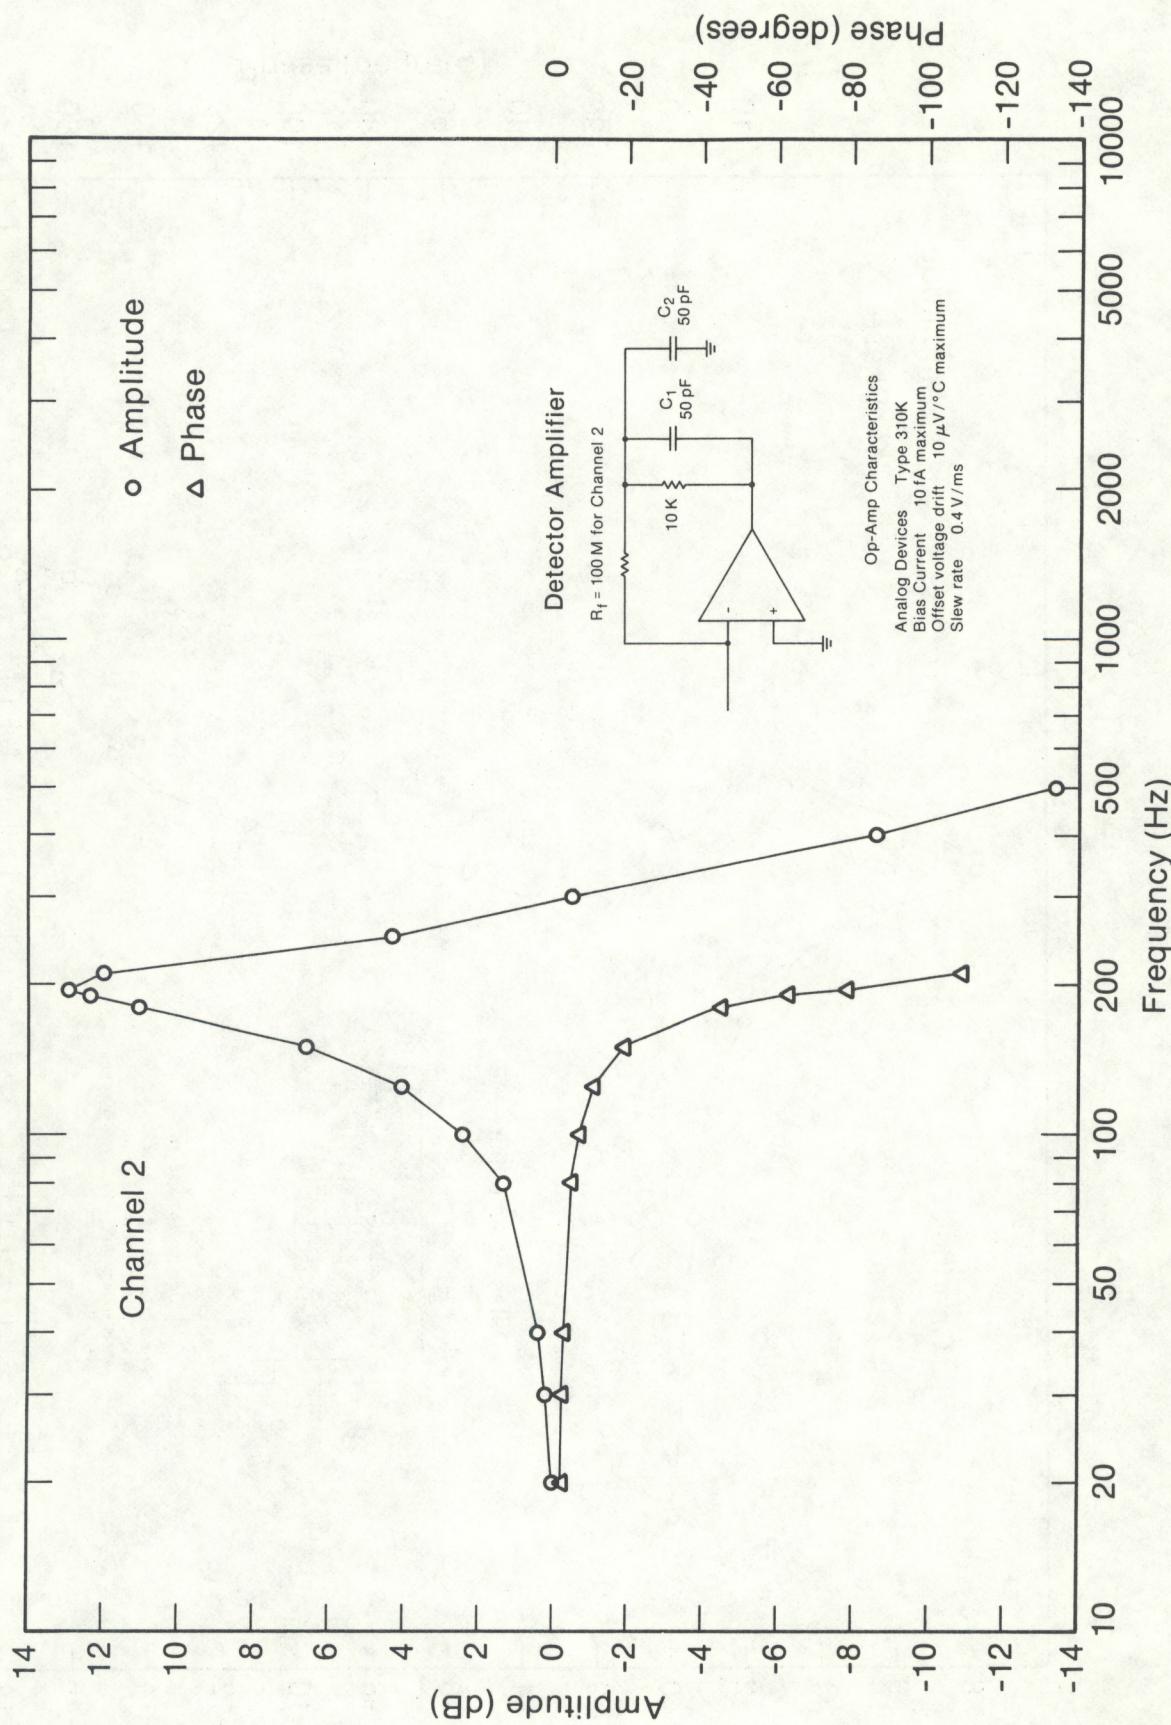


Fig. 5.—Amplitude and phase response of channel 2 of Buck's experimental hygrometer.

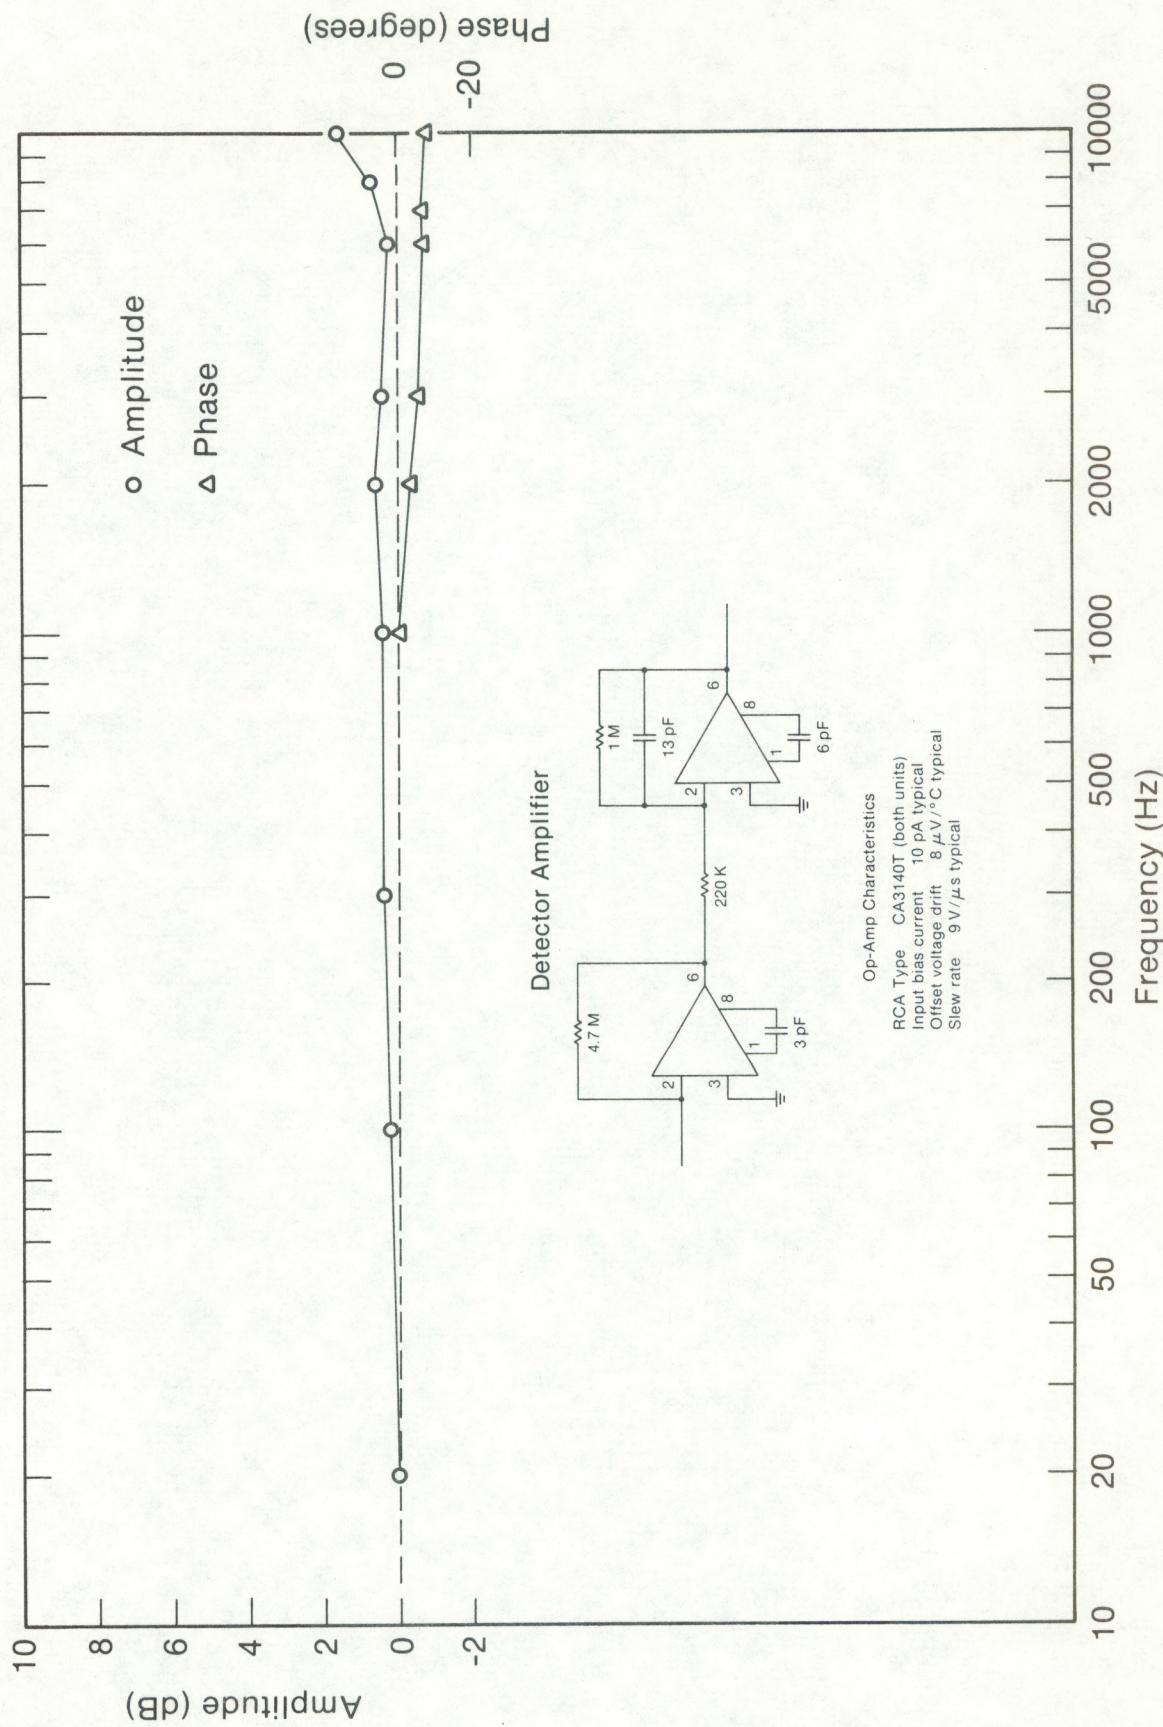


Fig. 6.—Amplitude and phase response of a humidimeter with an improved detector amplifier.